


Data file: D:\CHEM32\1\DATA\230726\800034_23072604FianI.D
 Sample name: 800034_23072604FianI
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 18-28% B in 20min, Flow rate: 1ml/min
 Column: Uni tary C18, 4.6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 36
 Injection date: 2023/7/26 14:13:03 Injection: 1 of 1
 Last changed: 2023/7/26 16:08:50 Injection volume: 10.000
 Acq. operator: SYSTEM

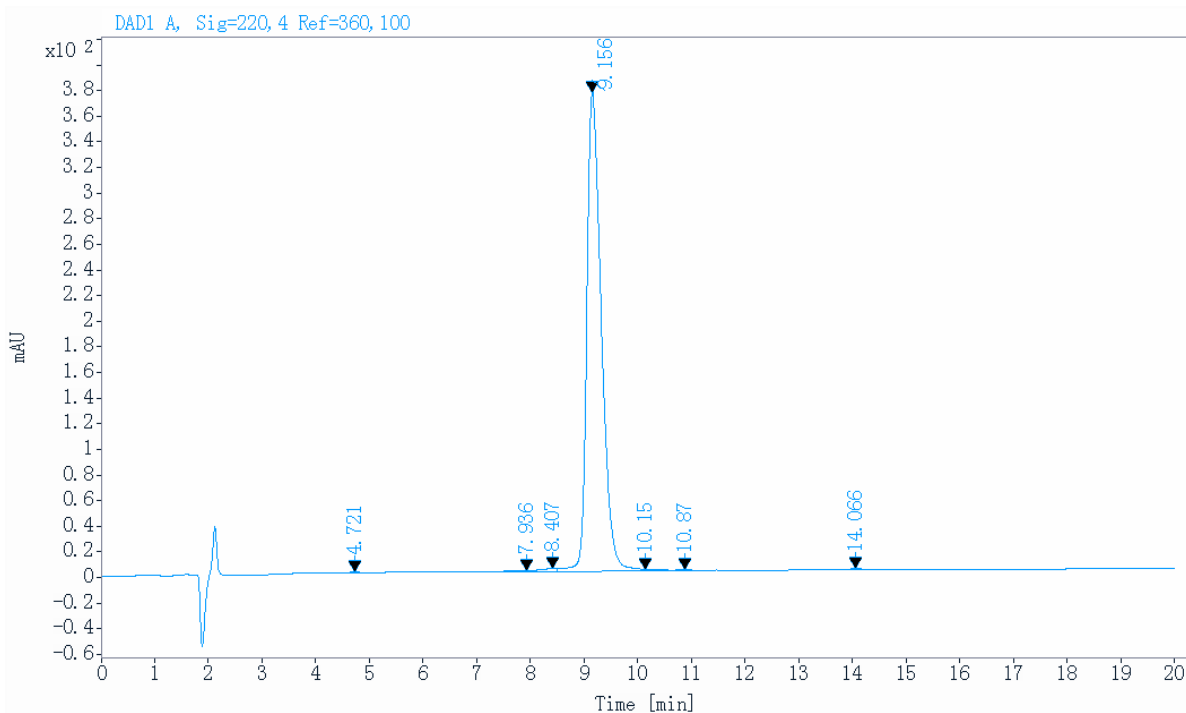

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
4.721	BB	0.1886	9.9025	0.7989	0.1386
7.936	MF	0.4090	24.4665	0.9971	0.3425
8.407	FM	0.3189	42.2806	2.2095	0.5919
9.156	MF	0.3125	7016.7534	374.2447	98.2229
10.150	MF	0.2410	20.0064	1.0307	0.2801
10.870	FM	0.3878	10.1179	0.4348	0.1416
14.066	VV	0.2963	20.1790	1.0314	0.2825
	Sum		7143.7063		